

# TEST REPORT

(Electronic version)



No: 200099299

VERIFICATION WEBSITE: [www.gttc.net.cn](http://www.gttc.net.cn)

VERIFICATION CODE: PAJI-3706-54

ISSUE DATE: 2020-05-11

二维码载报告



APPLICANT: ZHANGZHOU YUANLI BIOTECHNOLOGY CO., LTD  
ADDRESS: NO.10, LONGCHI AVENUE, JIAOMEI TOWN, ZHANGZHOU TAIWANESE INVESTMENT ZONE, FUJIAN

INFORMATION CONFIRMED BY APPLICANT:

3D FOLDING KN95 MASK

QUANTITY: SEVENTY PIECES

DATE RECEIVED/DATE TEST STARTED: 2020-04-26

CONCLUSION:

VISUAL FIELD	M
FILTRATION EFFICIENCY TO NaCl PARTICULATE MATTER	M
INSPIRATORY RESISTANCE	M
EXPIRATORY RESISTANCE	M
FLAMMABILITY	M
HEAD BAND	M
APPEARANCE INSPECTION[2 PIECES]	M

NOTE: "M" -MEET THE STANDARD'S REQUIREMENT "F" -FAIL TO MEET THE STANDARD'S REQUIREMENT  
"---" -NO COMMENT

REMARK:

THE AUTHORIZATION OF APPEARANCE INSPECTION IS NOT RECEIVED FROM CNAS.  
THIS REPORT IS THE ENGLISH TRANSLATION VERSION OF THE REPORT 200090222.  
ALL THE TESTED ITEMS ARE TESTED UNDER THE STANDARD CONDITION (EXCEPT FOR INDICATION).  
COPIES OF THE REPORT ARE VALID ONLY RE-STAMPED.  
THE EXPERIMENT WAS CARRIED OUT AT No.1, ZHUJIANG ROAD, PANYU DISTRICT, GUANGZHOU, GUANGDONG, P. R. CHINA.

APPROVED BY:

ZiShan Guo SENIOR ENGINEER

郭子山




PAGE 1 OF 4

# TEST REPORT

(Electronic version)

No:200099299

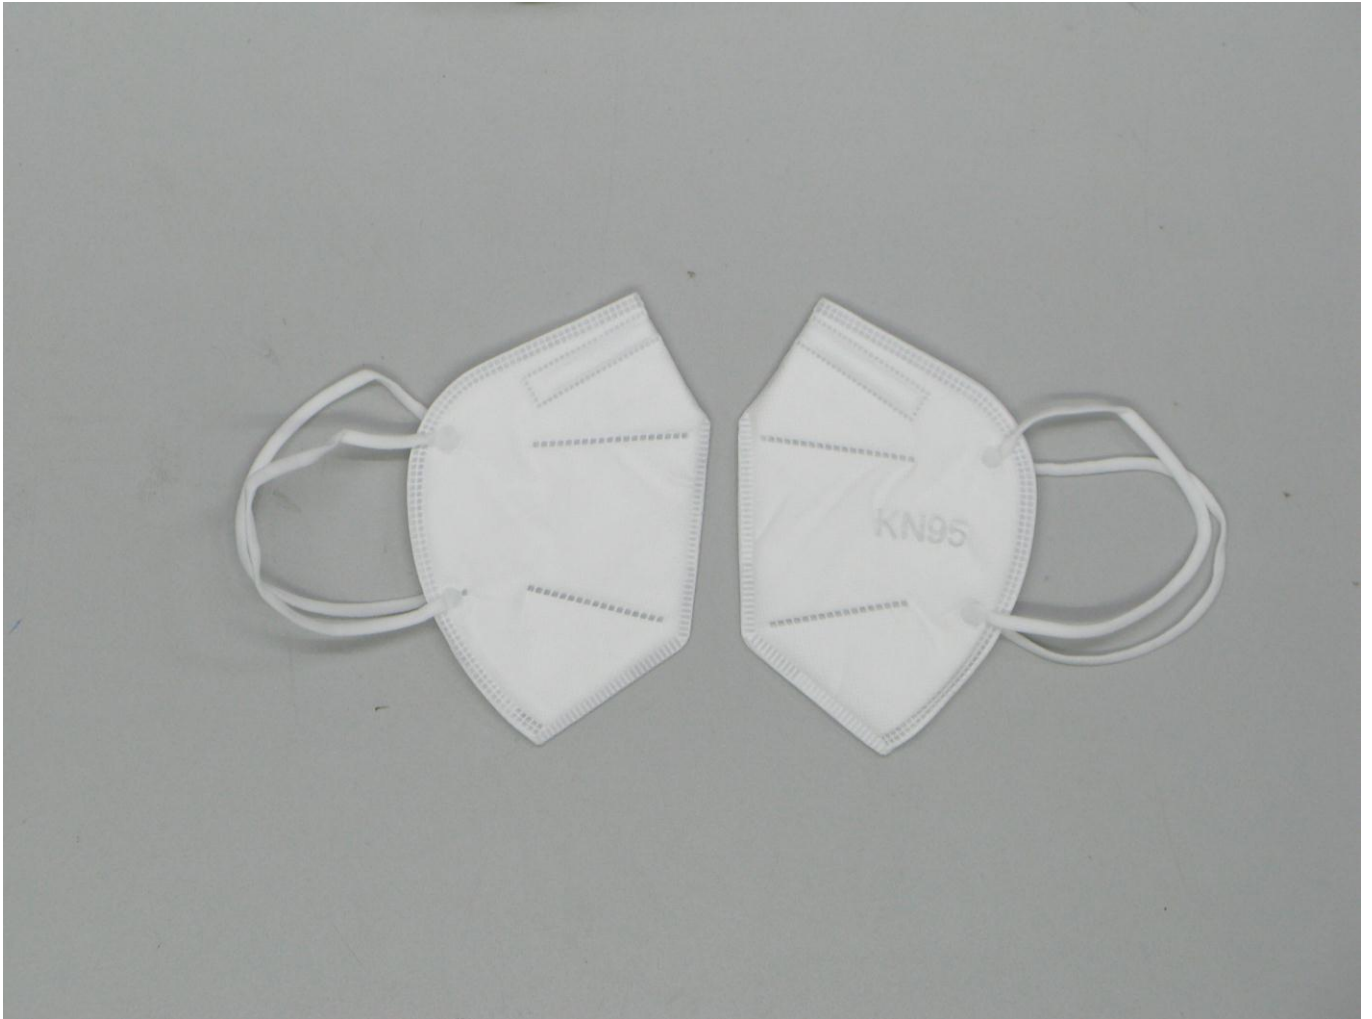

# TEST REPORT

(Electronic version)

No:200099299

## VISUAL FIELD(° )

(GB 2890-2009 6.8)

70

REQUIREMENT

≥60

(GB 2626-2006)

## FILTRATION EFFICIENCY TO NaCl PARTICULATE MATTER(%)

(GB 2626-2006 6.3, AIR FLOW:85L/min, AEROSOL:NaCl, AEROSOL CONCENTRATION:15mg/m<sup>3</sup>,  
TEMP:22.6℃ RH:36.9%)

FILTRATION EFFICIENCY:

UNTREATED SAMPLE

1# 98.82

2# 98.96

3# 98.70

4# 98.47

5# 98.87

6# 98.40

7# 98.32

8# 98.75

9# 98.18

10# 98.59

CONDITIONING TREATED

1# 98.36

2# 98.07

3# 97.86

4# 97.90

5# 98.27

REQUIREMENT

FILTRATION EFFICIENCY:

≥95.0

(KN95)

(GB 2626-2006)

## INSPIRATORY RESISTANCE (Pa)

(GB 2626-2006 6.5, HEAD SIZE: MEDIUM)

UNTREATED SAMPLE:

1# 129.8

2# 166.3

PRETREATMENT SAMPLE:

1# 116.7

2# 116.8

REQUIREMENT

≤350

(GB 2626-2006)

## EXPIRATORY RESISTANCE (Pa)

(GB 2626-2006 6.6, HEAD SIZE: MEDIUM)

UNTREATED SAMPLE:

1# 108.6

2# 147.3

PRETREATMENT SAMPLE:

1# 98.5

2# 100.1

REQUIREMENT

≤250

(GB 2626-2006)



PAGE 3 OF 4

# TEST REPORT

(Electronic version)

No:200099299

---

## FLAMMABILITY(s)

(GB 2626-2006 6.15)

AFTERFLAME TIME  
UNTREATED SAMPLE  
1# 0.0  
2# 0.0  
CONDITIONING TREATED  
3# 0.0  
4# 0.0

REQUIREMENT  
AFTERFLAME TIME  
≤5  
(GB 2626-2006)

---

## HEAD BAND

(GB 2626-2006 6.11)

UNTREATED SAMPLE:  
1# PASS  
CONDITIONING TREATED:  
1# PASS

REQUIREMENT  
EACH HEAD BAND, BUCKLE AND OTHER ADJUST  
PARTS OF MASK SHOULD NOT SLIP OR BREAK  
UNDER 10N TENSION FOR 10S.  
(GB 2626-2006)

---

## APPEARANCE INSPECTION[2 PIECES]

(GB 2626-2006 6.1)

PASS

REQUIREMENT  
ACCORDING TO THE CLAUSE 5.2 OF THE  
PRODUCT STANDARD  
(GB 2626-2006)

---



—End of Report—

PAGE 4 OF 4